

Application Bulletin

DEIONIZED WATER



Years ago, high purity water was used only in limited applications. Today, deionized (DI) water has become an essential ingredient in hundreds of applications including: medical, laboratory, pharmaceutical, cosmetics, electronics manufacturing, food processing, plating, countless industrial processes, and even the final rinse at the local car wash.

THE DEIONIZATION PROCESS

The vast majority of dissolved impurities in modern water supplies are ions such as calcium, sodium, chlorides, etc. The deionization process removes ions from water via ion exchange. Positively charged ions (cations) and negatively charged ions (anions) are exchanged for hydrogen (H⁺) and hydroxyl (OH⁻) ions, respectively, due to the resin's greater affinity for other ions. The ion exchange process occurs on the binding sites of the resin beads. Once depleted of exchange capacity, the resin bed is regenerated with concentrated acid and caustic which strips away accumulated ions through physical displacement, leaving hydrogen or hydroxyl ions in their place.

DEIONIZER TYPES

Deionizers exist in four basic forms: disposable cartridges, portable exchange tanks, automatic units, and continuous units. A two-bed system employs separate cation and anion resin beds. Mixed-bed deionizers utilize both resins in the same vessel. The highest quality water is produced by mixed-bed deionizers, while two-bed deionizers have a larger capacity. Continuous deionizers, mainly used in labs for polishing, do not require regeneration.

TESTING DI WATER QUALITY

Water quality from deionizers varies with the type of resins used, feed water quality, flow, efficiency of regeneration, remaining capacity, etc. Because of these variables, it is critical in many DI water applications to know the precise quality. Resistivity/conductivity is the most convenient method for testing DI water quality. Deionized pure water is a poor electrical conductor, having a resistivity of 18.2 million ohm-cm (18.2 megohm) and conductivity of 0.055 microsiemens. It is the amount of ionized substances (or salts) dissolved in the water which determines water's ability to conduct electricity. Therefore, resistivity and its inverse, conductivity, are good general purpose quality parameters.

Because temperature dramatically affects the conductivity of water, conductivity measurements are internationally referenced to 25°C to allow for comparisons of different samples. With typical water supplies, temperature changes the conductivity an average of 2%/°C, which is relatively easy to compensate. Deionized water, however, is much more challenging to accurately measure since temperature effects can approach 10%/°C! Accurate automatic temperature compensation, therefore, is the "heart" of any respectable instrument.

RECOMMENDED INSTRUMENTATION

Portable instruments are typically used to measure DI water quality at points of use, pinpoint problems in a DI system, confirm monitor readings, and test the feed water to the system. The handheld Myron L[®] Company instruments have been the first choice of DI water professionals for many years. For two-bed DI systems, there are several usable models with displays in either microsiemens or ppm (parts per million) of total dissolved solids. The most versatile instruments for DI water are the Ultrameter II™ 4P or 6PFC^E or Ultrameter III™ 9P, which can measure both ultrapure mixed-bed quality water and unpurified water. It should be noted that once DI water leaves the piping, its resistivity will drop because the water absorbs dissolved carbon dioxide from the air. Measuring of ultrapure water with a hand-held instrument requires not only the right instrument, but the right technique to obtain accurate, repeatable readings. Myron L[®] Company instruments offer the accuracy and precision necessary for ultrapure water measurements.

In-line monitor/controllers are generally used in the more demanding DI water applications. Increased accuracy is realized since the degrading effect of carbon dioxide on high purity water is avoided by use of an in-line sensor (cell). This same degradation of ultrapure water is the reason there are no resistivity calibration standard solutions (as with conductivity instruments). Electronic sensor substitutes are normally used to calibrate resistivity monitor/controllers.

Myron L[®] Company manufactures a variety of in-line instruments, including resistivity monitor/controllers which are designed specifically for DI water.

The 900 Series Multi-Parameter Monitor/Controller™ models simultaneously monitor and/or control multiple inputs and outputs. They are autoranging with 3 automatic temperature compensation standards for greatest accuracy (KCl, NaCl, and 442 Natural Water™). User adjustable temperature compensation (0 - 10%/°C) can be disabled for non-compensated readings. Input parameters include resistivity, conductivity, TDS, salinity, pH, ORP, flow/pulse and temperature. The Percent Rejection function of the 900 Series is designed to help quantify the effectiveness of water filtration systems. This is accomplished by comparing the feed water to the permeate (product) water to determine the percent of dissolved solids removed or rejected by the filtration system. The RS-485 serial output allows you to download data to a supervisory computer, PLC or SCADA system.

MYRON L[®]
COMPANY
Water Quality Instrumentation
Accuracy • Reliability • Simplicity

which can be used to control alarm(s), valve(s), pump(s), etc.

The 750 Series II in-line monitor/controllers offer seven resistivity ranges to suit any DI water application. A variety of options and outputs are available to cost-effectively tailor the monitor/controller to your particular application. Temperature compensation is automatic and achieved via a dual thermistor circuit.

Sensors are available constructed in either 316 stainless steel or titanium. All sensors are provided with a 3/4" MNPT polypropylene bushing and 10 ft./3 meters of cable. Optional PVDF or stainless steel bushings can be ordered, as well as longer cable lengths up to 100 ft./30 meters.


All Myron L® monitor/controller models contain adjustable set point(s), remote alarm connector(s) and heavy-duty relay(s)

The following table briefly covers some of the Myron L® Company instruments for DI water applications. For details and recommendations, please contact your local distributor, refer to Myron L® data sheets, visit our website (www.myronl.com), or contact us by phone, fax, or email (sales@myronl.com).

INSTRUMENT	PARAMETER	DI SYSTEM			
		Two Bed, Weak Base Anion 20-50 kΩ (50-20 μS)	Two Bed, Strong Base Anion 50-200 kΩ (20-5 μS)	Two Bed, Strong Base Anion 0.05-2.0 MΩ (20-0.5 μS)	Mixed Bed 1-18.23 MΩ (1-0.055 μS)
Handheld Instruments					
Ultrameter III™ 9P (Digital)	Multi-Parameter	x	x	x	x
Ultrameter II™ 6PFC ^E (Digital)	Multi-Parameter	x	x	x	x
Ultrameter II™ 4P (Digital)	Conductivity/TDS/Resistivity	x	x	x	x
Ultrapen™ PT1, PTBT1 (Digital)	Conductivity/TDS	x	x		
DS Meter™ 532M1 (Analog)	Conductivity	x	x		
DS Meter™ EP-10 (Analog)	Conductivity	x	x		
DS Meter™ EP (Analog)	Conductivity/Resistivity	x	x	x	x
In-line Instruments					
900M-3C Touchscreen Controller	Multi-Parameter	x	x	x	x
900M-1C Touchscreen Controller	Multi-Parameter	x	x	x	x
753II-XX Digital Controller*	Resistivity	x	x	x	x
758II-XXX Digital Controller*	Conductivity	x	x	x	x

* Range is specified at time of ordering.

RESISTIVITY VS. CONDUCTIVITY

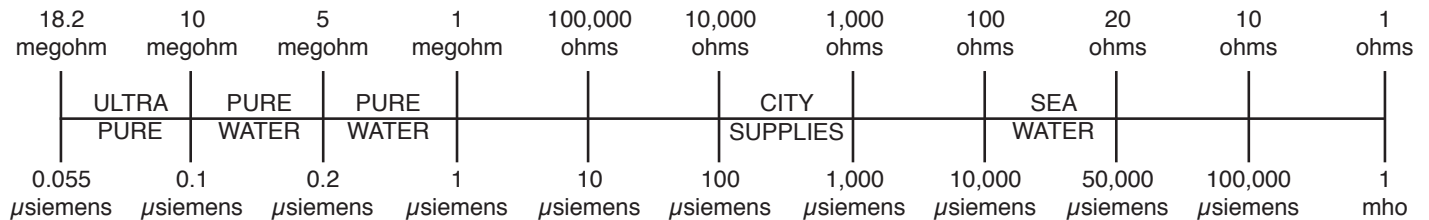

USEFUL CONVERSIONS

$$\frac{1}{\text{megohm}} = \text{microsiemens (micromho)} \quad \frac{1}{\text{microsiemens (micromho)}} = \text{megohm}$$

Examples: 1 micromho (μmho) = 1 microsiemen (μS); 0.5 microsiemens = 2 megohms (2,000,000 ohms)
200 kilohm (200,000 ohms) = 0.2 megohm = 5 microsiemens

2450 Impala Drive
Carlsbad, CA 92010-7226 USA
Tel: +1-760-438-2021
Fax: +1-800-869-7668 / +1-760-931-9189
www.myronl.com

Built On Trust. Founded in 1957, the Myron L® Company is one of the world's leading manufacturers of water quality instruments. Because of our commitment to product improvement, changes in design and specifications are possible. You have our assurance any changes will be guided by our product philosophy: accuracy, reliability, and simplicity.

